

Certificate of Analysis




Website: <https://peptide.wumolab.com/>

Contact at peptide@wumolab.com


Product Name	AHK-Cu 50 mg/vial	Received Date	September 18, 2026
Batch No.	WM-Q3F0-AU50	Reported Date	September 19, 2026
Brand	ANMIT LABS	Manufacturer	SUZHOU XILIN TECHNOLOGY CO.,LTD
Sample description	Blue lyophilized powder in labeled vial	Tests requested	Identity and purity assessment of peptide vial sample

Specification	Result	Method	Status
Identity	AHK-Cu	ESI-MS	✓ Conforms
Fill Amount / Label Claim	50 mg/vial	Filling Record	✓ Conforms
Purity	99.67%	RP-HPLC (220 nm)	✓ Conforms

HPLC Chromatogram (Retention Time: 2.953 min)

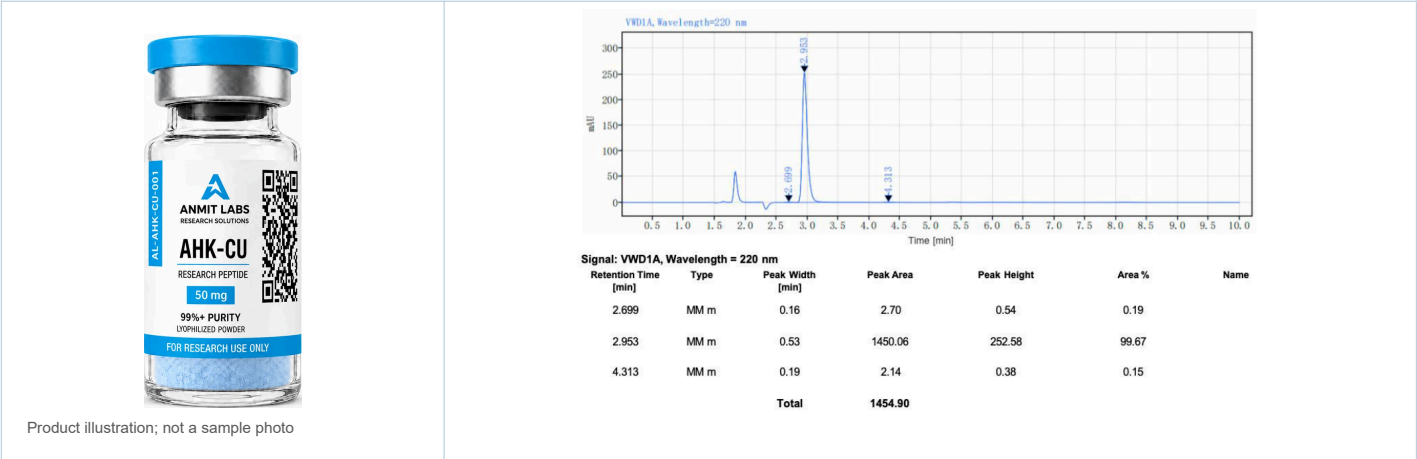

Mass Spectrum (ESI-MS)

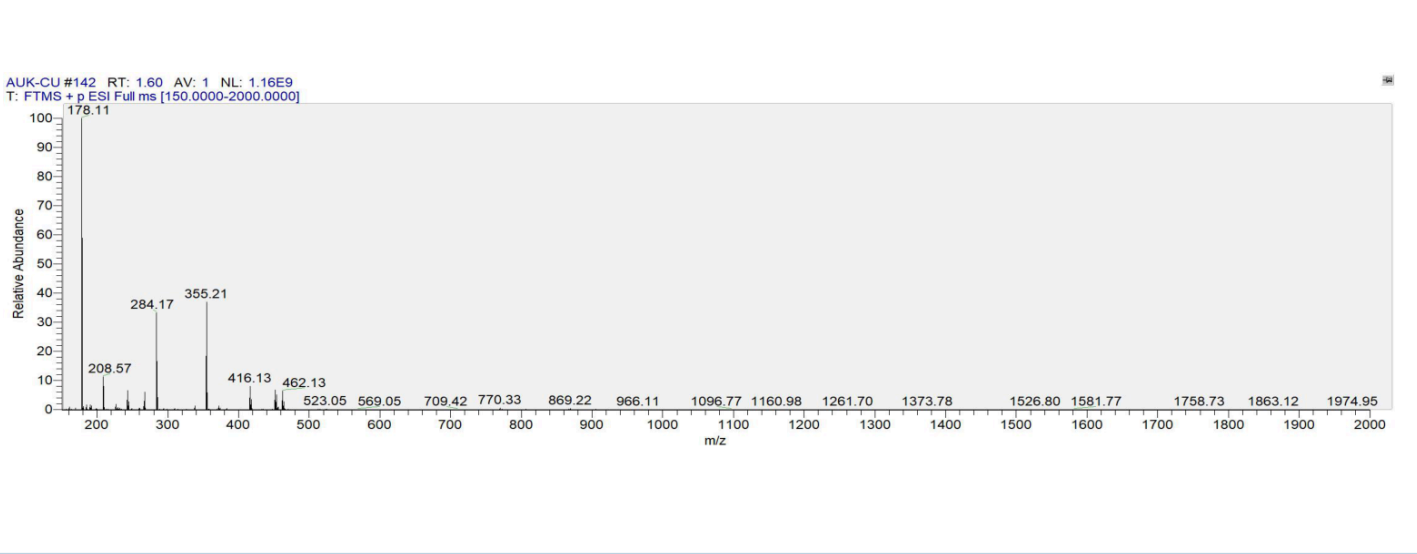

Remarks: For laboratory research use only. Not for human or veterinary use.

Checked By 	This report summarizes the test results for the submitted sample. Purity was analyzed by RP-HPLC, and identity was assessed by ESI-MS. The results apply only to the tested batch/sample and are provided for research and quality-control reference only.
---	--