

Certificate of Analysis




Website: <https://peptide.wumolab.com/>

Contact at peptide@wumolab.com


Product Name	Retatrutide 10mg/vial	Received Date	September 2, 2026
Batch No.	WM-U5O3-RT10	Reported Date	September 14, 2026
Brand	ANMIT LABS	Manufacturer	SUZHOU XILIN TECHNOLOGY CO.,LTD
Sample description	White lyophilized powder in labeled vial	Tests requested	Identity and purity assessment of peptide vial sample

Specification	Result	Method	Status
Identity	Retatrutide	ESI-MS	✓ Conforms
Fill Amount / Label Claim	10 mg/vial	Filling Record	✓ Conforms
Purity	99.87%	RP-HPLC (220 nm)	✓ Conforms

HPLC Chromatogram (Retention Time: 16.408 min)

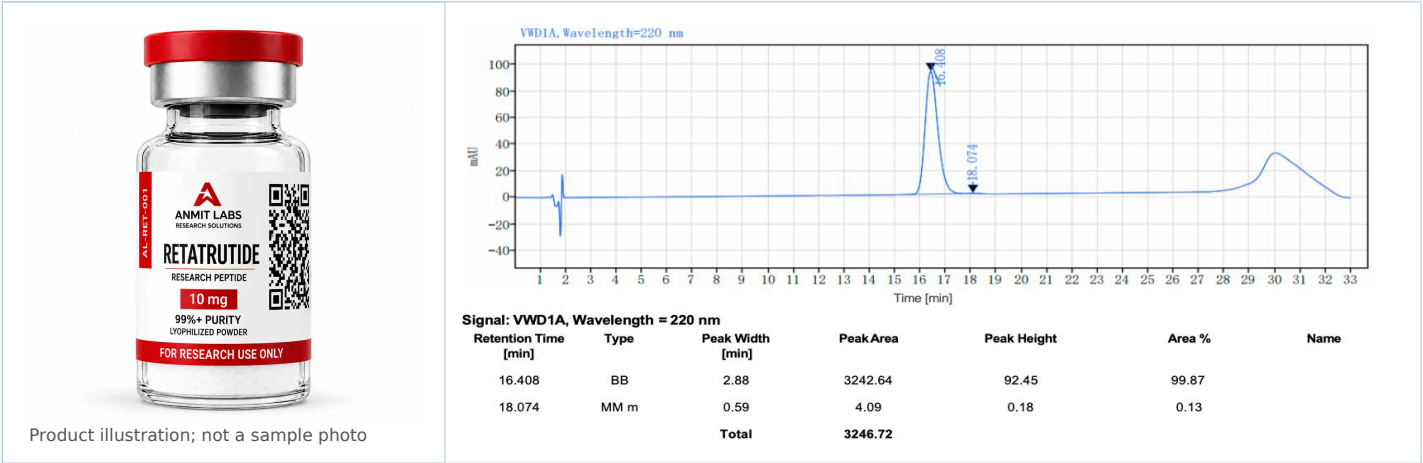

Mass Spectrum (ESI-MS)

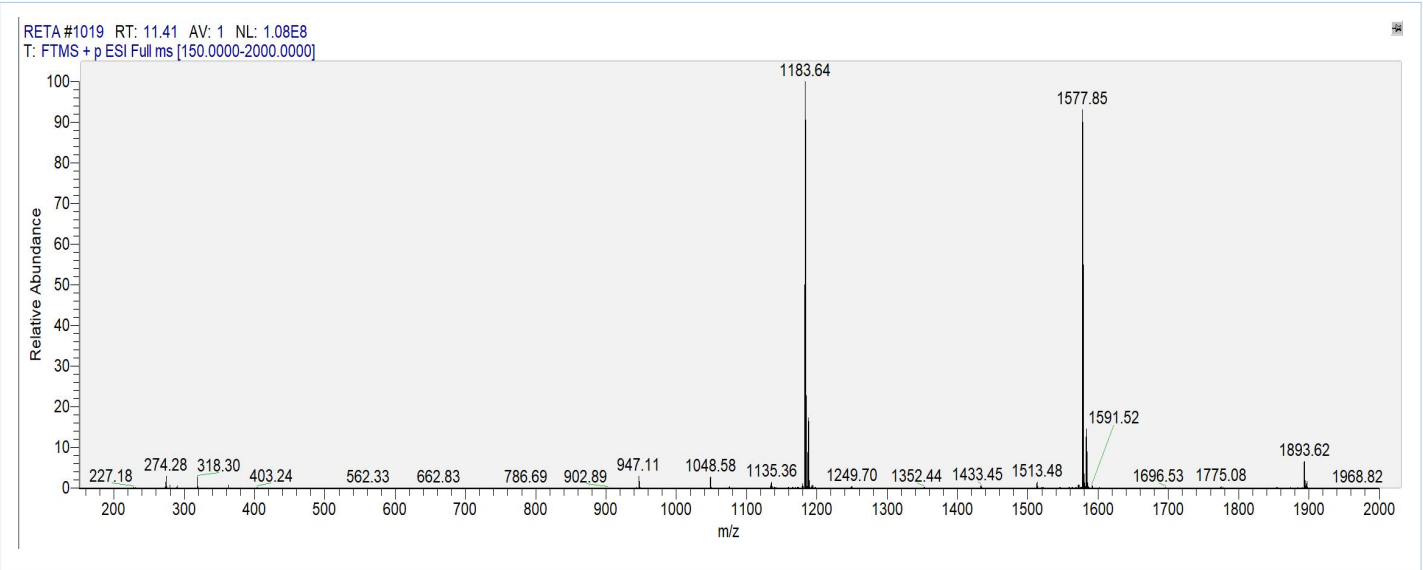

Remarks: For laboratory research use only. Not for human or veterinary use.

Checked By 	This report summarizes the test results for the submitted sample. Purity was analyzed by RP-HPLC, and identity was assessed by ESI-MS. The results apply only to the tested batch/sample and are provided for research and quality-control reference only.
----------------	--